


**FIG. 1**

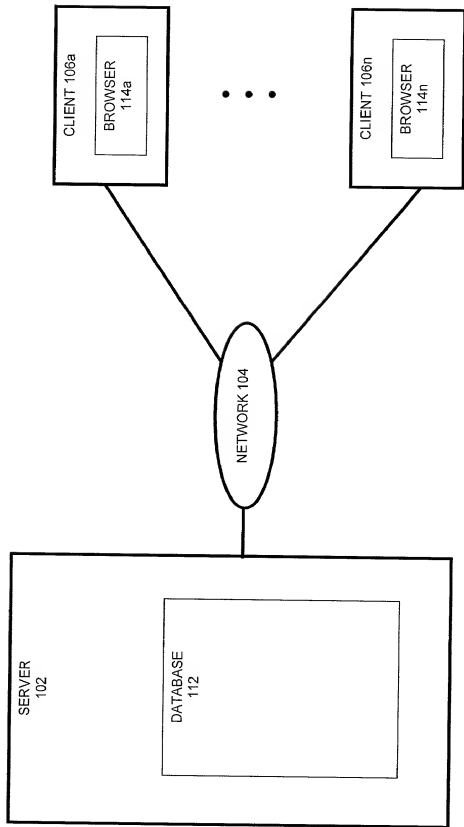

**FIG. 2**

SERVER  
102

MEMORY  
200

TRAINING PROGRAM  
202

OPERATING SYSTEM  
204

BUS 216

DATABASE  
206


ROM  
208

RAM  
210

CPU  
212

NETWORK  
INTERFACE  
214

09739357-121900

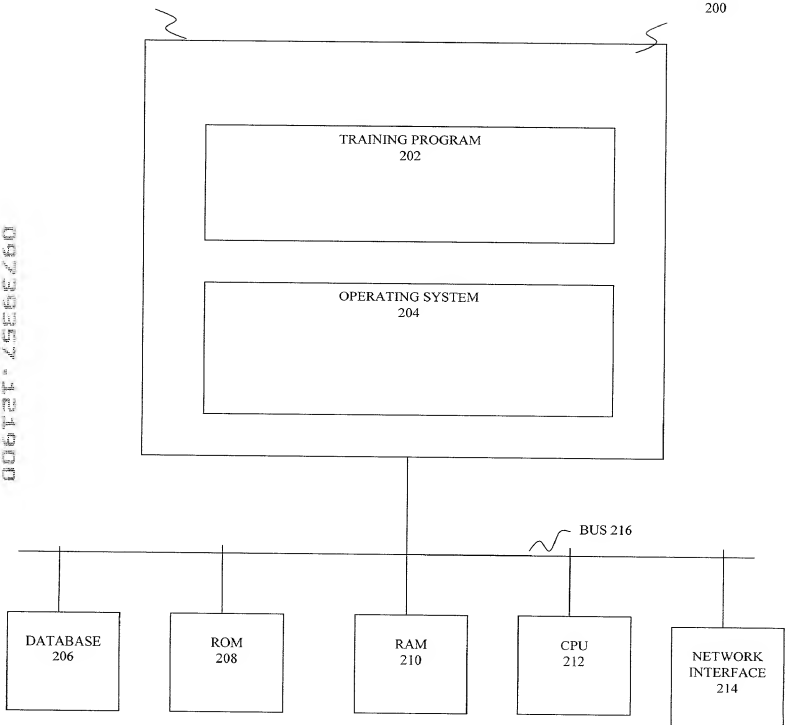

**FIG. 3**

USER COMPUTER 106

MEMORY 302

BROWSER PROGRAM  
304

OPERATING SYSTEM  
306

BUS 318

ROM  
308


RAM  
310

DISPLAY  
INTERFACE  
312

CPU  
314

NETWORK  
INTERFACE  
316

006121-2568260

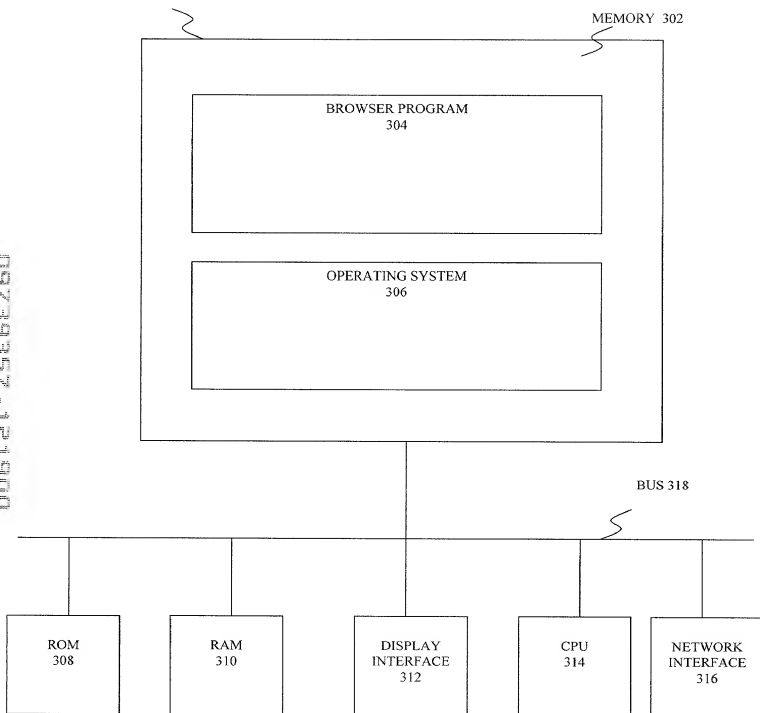

**FIG. 4**



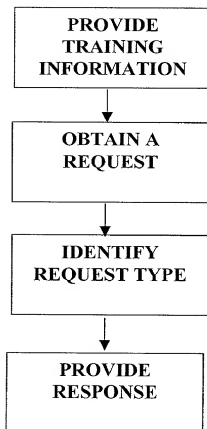


FIG. 5

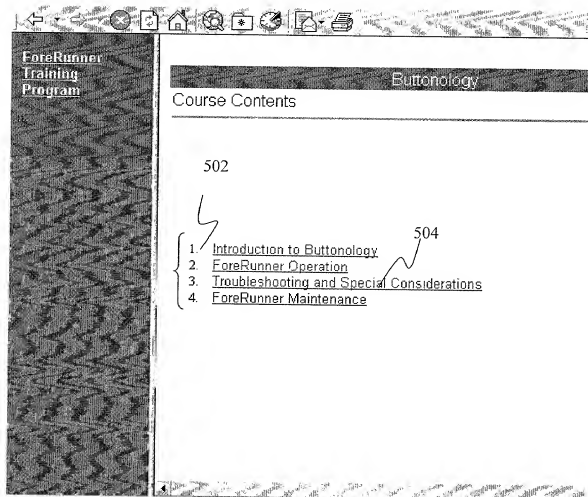

# FIG. 6

600

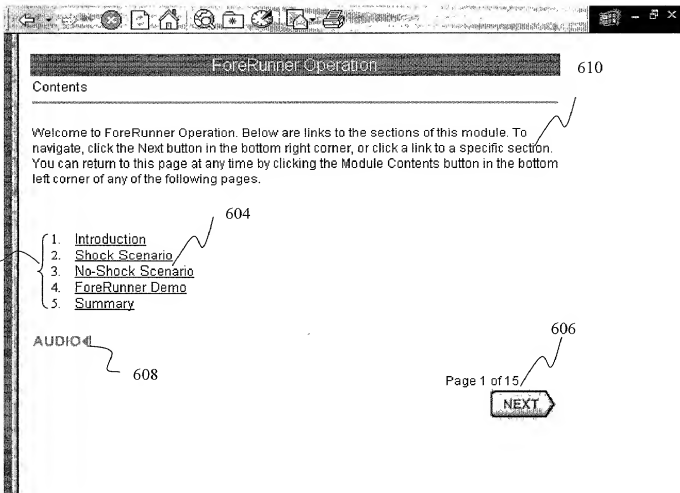

# FIG. 7

700

09739357.121900


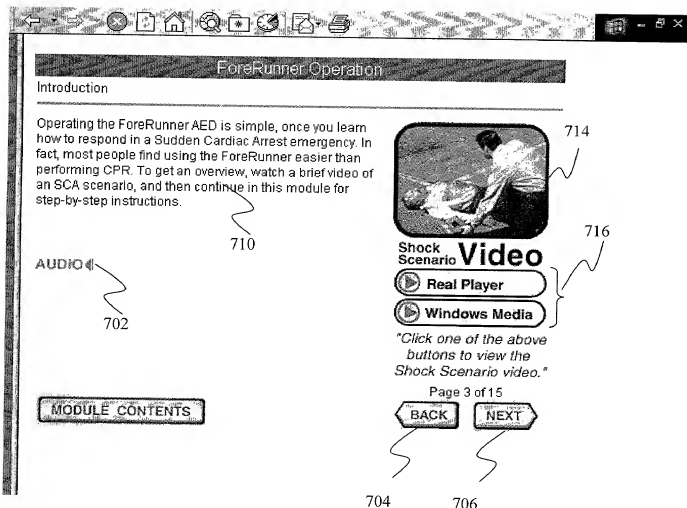


FIG. 8


800



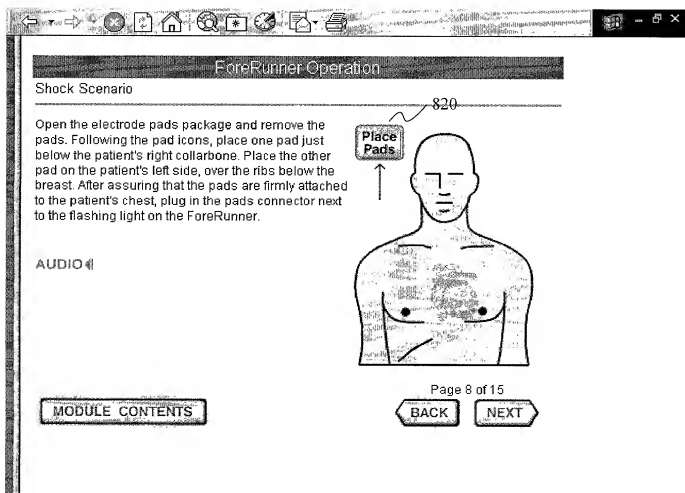

# FIG. 9

900

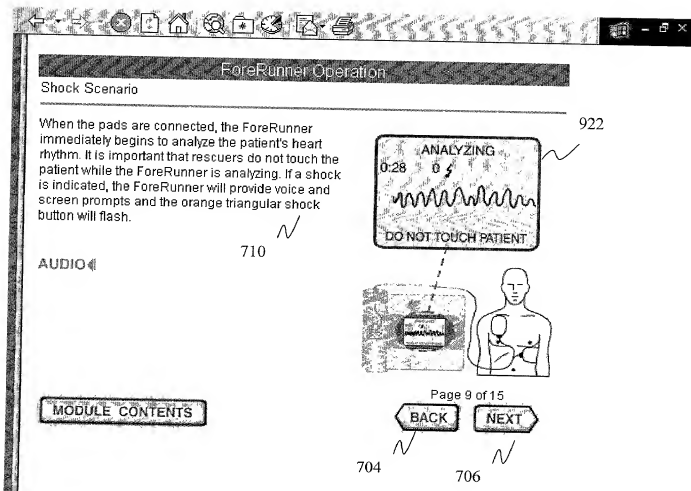

09739357.121900

**FIG. 10**

**1000**

09739357.121900


ForeRunner Operation

Shock Scenario

Before delivering the shock, it is important that the ForeRunner operator visually and verbally clears the patient. The ForeRunner operator should shout, "I'm clear," "you're clear," or simply "clear." Visually check to be certain that no one is touching the patient.

710

1518



After making sure everyone is clear of the patient, press the orange button to deliver the shock.

1024

AUDIO

MODULE CONTENTS

Page 10 of 15

BACK NEXT

# FIG. 11

1100

